



# Relax Order Form

**TO ORDER:**<https://eshop.jobst-ca.com>Email: [ca.elvarex@essity.com](mailto:ca.elvarex@essity.com)

Phone: 1.877.358.2739 | 1.877.978.5526

Fax: 1.877.978.9703

Patient Name / Essity File # \_\_\_\_\_ DOB \_\_\_\_\_ Date \_\_\_\_\_

Address \_\_\_\_\_ Gender M  F 

City/Province/Postal Code \_\_\_\_\_

Diagnosis \_\_\_\_\_

<b>PO#</b>	
Original Order <input type="checkbox"/>	Reorder w Changes <input type="checkbox"/>
Exact Reorder <input type="checkbox"/>	Schema # _____

Fitter Name _____	Fitter # _____	Fitter Phone _____
Fitter Facility _____	Fitter email _____	

Ship To Acct # _____	Acct Name _____
Address _____	City _____ Province _____ Postal Code _____
Email* _____	Phone _____ FAX _____
<small>*By choosing communication via email (above), I acknowledge that Personal Health Information associated with this purchase may be transmitted from BSN in a non-encrypted manner.</small>	

Bill To Acct # _____	Acct Name _____
Address _____	City _____ Province _____ Postal Code _____
Email _____	Phone _____ FAX _____

**Armsleeves**

Colour	Style	Quantity/Class	CCL 1 (15-20 mmHg*)
<input type="checkbox"/> Beige	<input type="checkbox"/> CG Armsleeve	Left	
<input type="checkbox"/> Rose	<input type="checkbox"/> AG Armsleeve w/gauntlet	Right	


**Lower Extremities**

Colour	Style	Quantity/Class	CCL 1 (15-20 mmHg*)	CCL 2 (20-30 mmHg*)
<input type="checkbox"/> Beige	<input type="checkbox"/> Knee High	Left		
<input type="checkbox"/> Rose	<input type="checkbox"/> Thigh High	Right		

**Comments**

## Measuring Guidelines

- 0 no tension
- + light tension
- ++ heavy tension

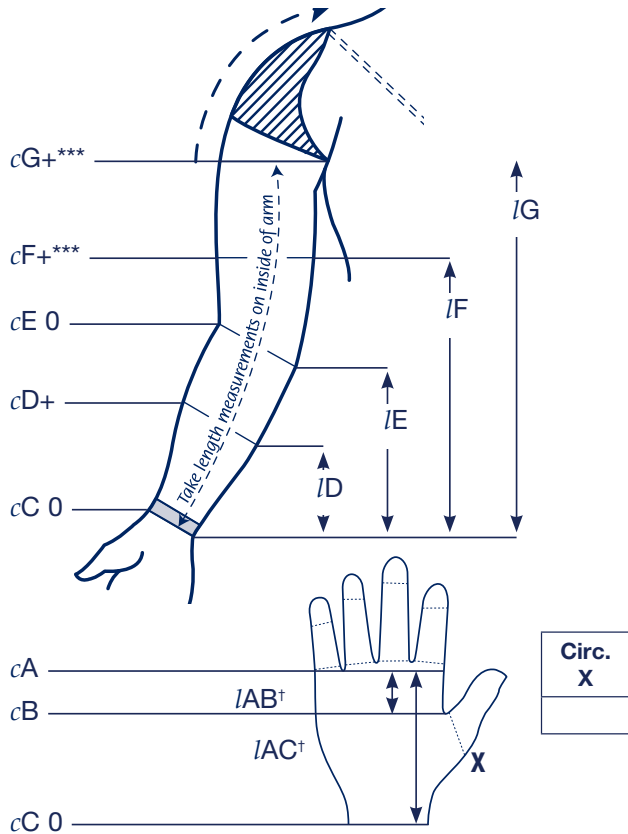

Circumference (c)	Length (l) Taken from inside of arm			
	Left	Right	Left	Right
cG+***			IG	
cF+***			IF	
cE 0			IE	
cD+			ID	
cC 0			IAB†	
cA			IAC†	
cB				

Circumference (c)	Length (l) Taken from each landmark to floor			
	Left	Right	Left	Right
cG+***			IG	
cF+***			IF	
cE+			IE	
cD+			ID	
cC++			IC	
cB'++			IB†	
cB+/0**			IB	
cY 0			IA	
cA+				

- \* Design Pressure
- \*\* If cB is <20cm, cB should be measured with 0 tension
- \*\*\* If needed, slightly more tension can be used
- † Add 1 cm to IAB and IAC